



IMAGING SYSTEM

VistARad Quick Start Guide

Version 3.0, Patch 115
February 2011 – Revision 9

Department of Veterans Affairs
Office of Enterprise Development
Health Provider Systems

**VistARad Quick Start Guide
VistA Imaging 3.0 Patch 115
February 2011**

Property of the US Government

This is a controlled document. No changes to this document may be made without the express written consent of the VistA Imaging development group.

While every effort has been made to assure the accuracy of the information provided, this document may include technical inaccuracies and/or typographical errors. Changes are periodically made to the information herein and incorporated into new editions of this document.

Product names mentioned in this document may be trademarks or registered trademarks of their respective companies, and are hereby acknowledged.

VistA Imaging Office of Enterprise Development

Department of Veterans Affairs

Internet: <http://www.va.gov/imaging>

VA intranet: <http://yaww.va.gov/imaging>

Contents

Introduction	v
Terms of Use	v
Getting Help	v
Getting Started	1
New Users.....	1
Returning Users	1
Starting & Exiting VistARad	2
Starting VistARad	2
How VistARad Windows Behave	2
Exiting VistARad.....	3
Locating & Opening Exams	4
Using the Manager Window	4
Opening Exams.....	5
Using ReadList.....	7
Working with Routed Exams.....	9
Surveying Exams	10
How VistARad Displays Exams.....	10
Images and Viewports.....	12
Conditional Indicator Icons.....	14
Navigating with Scouts	14
Navigating between Patients.....	15
Working with Images	16
Adjusting Images.....	16
Changing Layout in a Viewport.....	19
Changing Layout in a Window.....	19
Manipulating Image Sets.....	20
Mensurated Scale	21
Annotations	22
Key Images	26
Reviewing Online Records.....	27
Closing Exams	28
Hanging Protocols & Templates.....	29
Template & Hanging Protocol Basics.....	29
VistARad and Voxar 3D	31
Loading Images from VistARad into Voxar	31
Saving a Voxar Capture to VistA as a New Series.....	32
Teaching Files	33
Creating Teaching Files	33
VistARad and Voice Dictation	35
About the VistARad Dictation Interface.....	35
Opening Exams and Reports for Dictation.....	35
Remote Data/Image Views.....	37

Revision Table

Date	Rev	Notes
Feb 3 2011	9	Updates for Patch 115. J. Christensen, M. Turian, J. Kennedy.
Jun 8 2010	8	Updates for Patch 90. J. Christensen, M. Turian, J. Kennedy.
Mar 31 2010	7	Corrections related to packaging issues with graphics and links. J. Kennedy.
Dec 10 2009	6	Updates for Patch 101. J. Christensen, J. Kennedy.
Dec 03 2007	5	Remove non-essential p65 content. Reorganize <i>Surveying Exams</i> section. Updates for Patch 76. A. McFarren, J. Christensen.
Feb 21 2007	4	Updates for Patch 65. A. McFarren, J. Christensen.
April 3 2006	3	Updated for release of Patch 18. A. McFarren, J. Christensen.
Jun 20 2005	2	Pre-alpha draft. A. McFarren, J. Christensen.
May 23 2005	1	VEHU draft. A. McFarren, J. Christensen.

Introduction

This document is intended for radiologists and clinicians who use the VistARad diagnostic workstation. Information is included for new users about how to use key VistARad features. For returning users, a summary of changes in the most recent VistARad patch is provided, with an explanation of how those changes affect existing VistARad features.

It is assumed that:

- You are familiar with the Windows environment.
- The Patch 115 client is installed on a Windows XP-based diagnostic workstation, and the Patch 115 KIDS is installed on the VistA Host.
- Appropriate test exams are available.

Terms of Use

Use of the VistARad diagnostic workstation is subject to the following provisions:



Caution: Federal law restricts this device to use by or on the order of either a licensed practitioner or persons lawfully engaged in the manufacture or distribution of the product.



No modifications may be made to the VistARad diagnostic workstation without the express written consent of the VistA Imaging National Project Manager.



The Food and Drug Administration classifies the VistARad software as a medical device. Modifications to the VistARad diagnostic workstation, such as the installation of unapproved software, will adulterate the medical device. The use of an adulterated medical device violates US federal law (21CFR820).



Image presentation quality depends on monitor resolution, and on regular monitor testing and calibration to correct for display degradation over time. It is the responsibility of the clinical practitioner to determine if images presented on a VistARad workstation are of sufficient quality for clinical interpretation. Any concerns regarding monitor resolution or calibration should be reported immediately to the Imaging Coordinator before interpretation is performed.

Getting Help

If you encounter any problems using VistARad, contact your local Imaging Coordinator or support staff. If the problem cannot be resolved locally, use Remedy to place a service request, or contact CPS (Clinical Product Support) at 1-888-596-4357.

Getting Started

New Users

To learn how to use VistARad for basic exam interpretation, review the Basic Workflow topics listed below. For information about speeding up and fine-tuning interpretation, review the topics listed under Workflow Refinements.

Basic Workflow	See...	Workflow Refinements	See...
Log in	page 2	Use ReadList	page 6
Open an exam	page 5	Select a hanging protocol	page 6
Display patient records	page 27	Move, clone, split images	page 19
Survey exams	page 10	Annotate/measure images	page 22
Work with images	page 16	Change layout	page 19
Close an exam	page 28	Mark images	page 26

Returning Users

This table summarizes changes in Patch 115 that affect VistARad functionality. Places in this document that reference these changes are flagged with a “New in 115” sidebar.

Change	Details	See...
VOI LUT	Conditional indicator icons in the upper-right corner of images to alert you to certain conditions.	page 14
Scout images	Slice projection of intersecting images can now be used for images that have not been explicitly designated as scouts.	page 14
Line Measurement Button	Previously grouped with the angle measuring tools, now on the toolbar with its own dedicated icon	page 23
Teaching files	An entire series or study can now be sent to a MIRC server in one interaction.	page 33

Starting & Exiting VistARad

Starting VistARad

- 1 If VistARad has been integrated with a voice dictation system such as Talk or PowerScribe, log in to the voice dictation software.
- 2 Double-click the VistARad shortcut on the Windows desktop, or go to the Start menu and select **All Programs | VistA Imaging Programs | MAG_VistARad_Patch115**.






- 3 If the Connect To box displays, select which VistA System you want to connect to, then click **OK**.
- 4 In the VistA Sign-on box, enter your access and verify codes, then click **OK**. Keystrokes display as asterisks (*).
- 5 If the Select Division box displays, double-click the division you want to log in to.
- 6 When VistARad starts, both the Manager and Viewer windows open.

How VistARad Windows Behave

The Viewer window is designed to stretch across multiple monitors, and is usually not resized or minimized. Other VistARad windows can be sized, minimized, or 'tacked' into place as needed.





The Viewer

The buttons in the upper right corner of the Viewer work as follows:

-  Clicking this button minimizes the Viewer window.
-  This button is disabled.
-  Clicking this button exits VistARad.

Other VistARad windows

Except for the Viewer window, other VistARad windows have the following buttons in their upper right corners:

-  (or ) Clicking this button lets you control which windows stay visible while you are working with the Viewer, and which windows that you want 'out of the way' when you are not actively using them.
-  If present, clicking this button either maximizes the window to cover the entire screen or restores the window to its original size. This button is not available in the Preview, Scout, or Reports window.
-  Clicking this button minimizes the window.

Restoring minimized windows

Use one of the buttons in the Viewer window toolbar to restore minimized windows.



Alternatively, press <CTRL+W> or use the Windows taskbar to restore any window.

Exiting VistARad

- 1 Go to the menu bar in either the Manager or the Viewer and click **File | Exit VistARad**.
- 2 If the Close Exams/Update Status dialog displays, make sure the **Interpret?** and Annotation fields are set as desired for each exam in the dialog, then click **OK**. For details, see page 28.

Locating & Opening Exams

Using the Manager Window

The Manager window is used to locate and open exams and reports.

The screenshot shows the Manager window interface. At the top, there are tabs for 'Exam List', 'Patient Lookup', 'Patient Exams', 'Exam History', 'Unread Exams', 'Custom', and 'All Active Exams'. The 'Unread Exams' tab is active, displaying a table of 40 unread exams. Below this table are buttons for 'Open With', 'Open', 'Open/No Prior', 'ReadList', 'Close Exams', 'Report', 'Requisition', 'Health Summary', 'Patient Profile', 'Next', and 'Stop Load'. At the bottom, there is a section for 'Open/Reserved Exams' showing a table of exams that have already been opened.

Case #	Lock	Patient Name	ID #	Priority	Procedure	Image Date/Time	Sta...	# Im
092602-123	IP8	IMAGPATIENT1011,1011	I1011	4-Rout	CT ABDOMEN W/CONT	09/26/2002@18:03	EX...	112
112403-176		IMAGPATIENT1201,1201	I1201	4-Rout	CHEST 2 VIEWS PA&LAT	11/24/2003@17:07	EX...	2
112403-175		IMAGPATIENT1201,1201	I1201	4-Rout	CT THORAX W/CONT	11/25/2003@09:43	EX...	66
112403-179		IMAGPATIENT1202,1202	I1202	4-Rout	CHEST 2 VIEWS PA&LAT	11/25/2003@10:30	EX...	2
112403-180		IMAGPATIENT1203,1203	I1203	4-Rout	SHOULDER 2 OR MORE ...	11/25/2003@10:40	EX...	6
112403-181		IMAGPATIENT1203,1203	I1203	4-Rout	MAGNETIC IMAGE,UPPER...	11/25/2003@10:53	EX...	93
112403-183		IMAGPATIENT1204,1204	I1204	4-Rout	ABDOMEN 3 OR MORE VL...	11/25/2003@11:08	EX...	4
112403-182		IMAGPATIENT1204,1204	I1204	4-Rout	CHEST 2 VIEWS PA&LAT	11/25/2003@11:19	EX...	2
112403-184		IMAGPATIENT1204,1204	I1204	4-Rout	CT ABDOMEN W/CONT	11/25/2003@11:27	EX...	113

Case #	Lock	Patient	Procedure	Load Status	HP Selected
092602-123	LOCKED	IMAGPATIENT1011,1011	CT ABDOMEN W/CONT	Displayed	CT Thorax_2-hd_SY
011401-91		IMAGPATIENT1011,1011	CT ABDOMEN W&W/O CONT	Displayed	CT Thorax_2-hd_SY
011401-92		IMAGPATIENT1011,1011	CT ABDOMEN W&W/O CONT	Displayed	CT Thorax_2-hd_SY

Exam lists, which are used to organize exams into manageable groups, are displayed as a row of tabs near the top of the Manager window. Many sites use customized exam lists to create specific groupings of exams. These lists, if available, can be viewed by clicking the Custom tab.

You can use the settings under **View | Settings | Manager | General** to show or hide exam lists. Some lists, such as the Unread Exams list, cannot be hidden.

Exam Locks and Exam Reserves

In VistARad, locks and reserves are used to prevent two radiologists from interpreting the same exam.

The screenshot shows the 'Unread Exams' tab active, displaying a table of 71 unread exams. The table includes columns for Case #, Lock, Patient Name, ID #, and Priority. Two specific rows are highlighted with callouts: one with a 'LOCKED' status and another with a 'Reserved' status.

Case #	Lock	Patient Name	ID #	Priority
020602-98	IP8	IMAGPATIENT1011,1011	I1011	2-Urg
061390-8	IP8:R	IMAGPATIENT1009,1009	I1009	4-Rout
052098-15		IMAGPATIENT1009,1009	I1009	4-Rout
052198-16		IMAGPATIENT1009,1009	I1009	4-Rout

Unless locks are explicitly disabled, unread exams are locked on a first come, first served basis—the exam is automatically locked in the name of the first radiologist to display an unread exam.

If a radiologist closes a locked exam without updating its status, the lock is removed, and the exam can be locked and interpreted by a different radiologist.

Exam reserves are a ‘pre-lock’ used for exams that have been loaded into memory as part of the ReadList process. A reserved exam is automatically locked when it is displayed.


For details about ReadList, see page 6.

Opening Exams

The following sections explain two of the most frequently used methods used to open an exam. For additional methods, see the *VistARad User Guide*.

Opening an Exam I


Use these steps to open an exam and to automatically select a hanging protocol. (Hanging protocols are described on page 29.)

- 1 Display the Manager window by clicking  in the Viewer toolbar.
- 2 In the Manager window, click the **Unread Exams** tab.
 - To open the selected exam in the list, click **Open** or press <ENTER>.
 - To open any exam in the list, select the exam you want to open, then double-click the exam, or click **Open**.
- 3 As the exam opens and images are loaded, additional prompts or windows may display:
 - Usually, the requisition for the exam displays automatically.
 - If more than one matching hanging protocol is found, you are asked to select which hanging protocol you want to use. For details, see page 30.
 - If the voice dictation interface of VistARad is enabled, the report for that exam automatically opens for dictation. For details, see page 35.

- If the exam being opened is locked, and if not all image sets are loaded in the Viewer window, the Preview window displays. For complex exams (such as CT and MR exams), the Preview window can be used to monitor and alter the order in which series are loaded. For details, see page [10](#).
- 4 Images in the Viewer can be interacted with as soon as they display. For more details about the Viewer, see page [10](#).

Opening an Exam II


Use these steps to open an exam using a manually selected hanging protocol. (Hanging protocols are described on page [29](#).)

- 1 Display the Manager window by clicking  in the Viewer toolbar.
- 2 In the Manager window, click the **Unread Exams** tab.
- 3 Select the exam you want to open.
- 4 Make sure the check box to the right of the **Open With** button is cleared.
- 5 Click **Open With**.
- 6 Use the dialog that opens to select a hanging protocol.
 - Hanging protocols are grouped under each username, and a default collection is available under the “sysAdmin” group.
 - The viewport arrangement of the selected hanging protocol is shown in the Preview area near the bottom of the dialog.
- 7 Select the hanging protocol or template you want to use, and click **OK**.
- 8 As the exam opens and images are loaded, additional prompts or windows may display:
 - Usually, the requisition for the exam displays automatically.
 - If the voice dictation interface with VistARad is enabled, the report for the exam automatically opens for dictation. For details, see page [35](#).
 - If the exam being opened is locked, and if not all image sets are loaded in the Viewer window, the Preview window displays. For details, see page [10](#).

Using ReadList

ReadList lets you successively display all unread exams in an exam list. When ReadList is active, you can step from one unread exam to the next in a single step, without displaying the Manager, and with minimal wait times.

Starting ReadList

- 1 Display the Manager window by clicking  in the Viewer toolbar.
- 2 In the Manager window, click the **Unread Exams** tab.
- 3 Click the **ReadList** button, located near the middle of the Manager window. This opens the first unread exam in the list.
 - A matching hanging protocol is selected automatically. If there are multiple matches, you are prompted to select the hanging protocol you want to use. For details, see page 30.
 - Any priors identified by the selected hanging protocol also open automatically.
- 4 The exam and any priors display. As you are reviewing the displayed exam, the next exam in the Unread list is reserved and loaded into memory. Any applicable priors are loaded as well.

Exams in Viewer (current exam and one prior).


Exams loaded in memory (current exam and three priors). These exams will be displayed as soon as preceding exam is closed.

Open/Reserved Exams				
Case #	Lock	Patient	Procedure	Load Stat
112403-222	LOCKED	IMAGPATIENT408,408	CT ABDOMEN W/CONT	Displayed
112403-221		IMAGPATIENT408,408	CT ABDOMEN W/CONT	Displayed
112403-220	RESERVED	IMAGPATIENT1208,1208	CHEST SINGLE VIEW	Loaded
112403-219		IMAGPATIENT1208,1208	CHEST SINGLE VIEW	Loaded
112403-218		IMAGPATIENT1208,1208	CHEST SINGLE VIEW	Loaded
112403-217		IMAGPATIENT1208,1208	CHEST 2 VIEWS PA&&L...	Loaded

Note If the voice dictation interface for VistARad is enabled, the report for the exam being opened displays in the voice dictation window. Save any findings you entered for that exam before the next exam in VistARad.

Stepping through Exams with ReadList

When ReadList is active, you can step through exams without using the Manager. When you are ready to close an exam, do the following:

- 1 If VistARad has been integrated with a voice dictation system, and if you have a report open in that system, save or sign the report.
- 2 In VistARad, press <CTRL + N>, click **Next** in the Manager, or click  in the Viewer toolbar. The Close Exams/Update Status dialog opens.
- 3 Set the values in the Close Exams/Update Status dialog as desired. For details, see page [28](#).
- 4 Click **OK** to close the Close Exams/Update Status dialog.
 - After the dialog is closed, the next exam in the ReadList sequence displays.
 - VistARad automatically refreshes the active exam list, and preloads and reserves the next exam in the list.
 - ReadList mode continues until all unread exams have been displayed or until ReadList is stopped manually.


Stopping ReadList Manually

To stop ReadList manually, click the **Stop RL** button located near the middle of the Manager window. (This button is only visible when ReadList is active.) The currently displayed exam remains open, but no additional exams open once the currently displayed exam is closed.

Working with Routed Exams

If your workstation is set up for remote reading, you can use VistARad to interpret copies of exams routed to you from other sites. Working with a routed exam that is temporarily stored on your workstation is much faster than retrieving that exam from the originating site.

When you log in to a site to read exams from a remote location, the Manager window displays the **Remote Read Filter** button and the **RC** column to indicate that routed exams may be present.

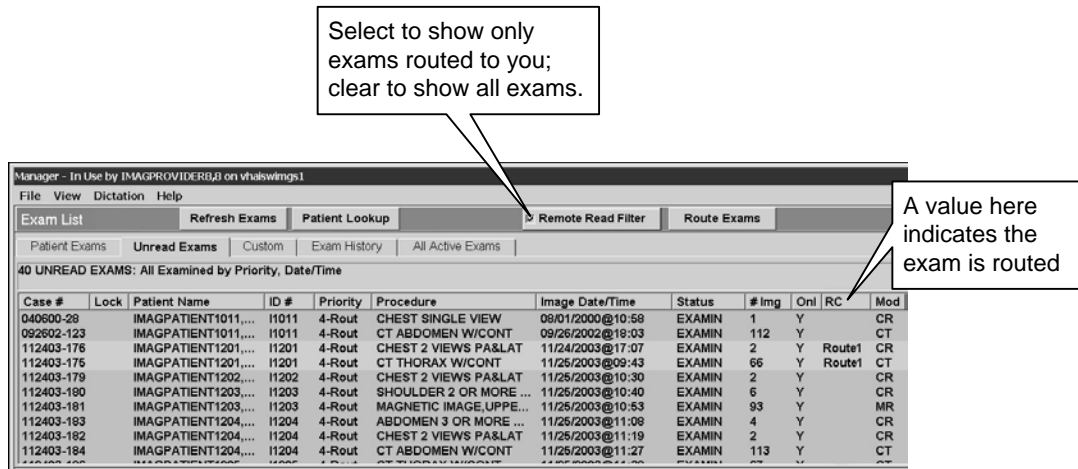

The process to open and interpret a routed exam is the same process used for non-routed exams. For information about opening exams, see page 5.

Certain settings control how VistARad manages prior exams and ReadList functions when routed exams are present. To review these settings, click **View | Settings** and select the **Remote/Local Reading** tab.


A VistARad workstation can also be set up to route exams on-demand. For details, see the *VistARad User Guide* or the *Routing User Guide*.

Surveying Exams

How VistARad Displays Exams


Once an exam has been opened using the Manager, images are generally loaded into the Preview and Viewer windows. Images can also be manually loaded into the Browser window.

The Preview Window


The Preview window provides a summary view of exams that are currently open. If the Preview window is not visible, it can be displayed by clicking  in the toolbar near the top of the screen.

Each exam in the Preview is shown as one or more thumbnail images, where each thumbnail represents an *image set* of one or more related images. General radiology (CR) exams are usually presented as a single image set. Cross-sectional (CT and MR) exams are usually presented as multiple image sets, with each thumbnail representing a series.

The Preview window tracks the display state of each image set in an open exam.

- If an  icon is displayed in the thumbnail, the associated image set is loaded and visible in the Viewer or the Browser.
- If a **P** icon is displayed in the thumbnail, the associated image set is partially loaded or was paused.
- If an **H** icon is displayed in the thumbnail, the images are loaded into the Viewer window but are hidden. For details, see page [13](#).
- If no icon is displayed in the thumbnail, the associated image set must be loaded manually.

In addition to the thumbnail view, the Preview window incorporates a “List view.” In List view, a set of progress bars shows the loading status of all exams. Using List view, you can pause or resume the load of series (image sets) within an exam. You can also purge image sets to free up memory.

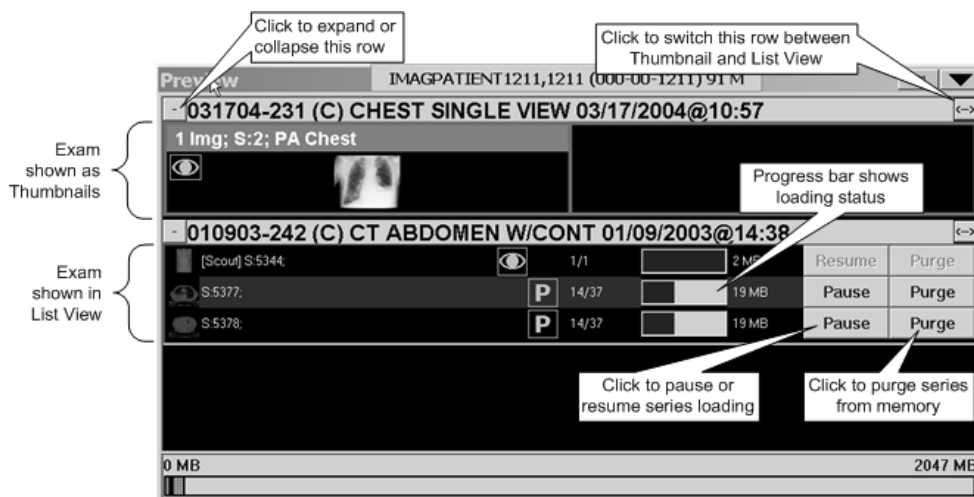

To load an image set manually

Drag the appropriate thumbnail from the Preview window into a viewport in the Viewer window. You can also double-click the thumbnail to display the entire exam in the Browser window. Each list view item, like the thumbnail, can be dragged onto the viewport.

The Viewer Window


The Viewer window occupies most of the display space on a VistARad workstation, and is the primary workspace for exam interpretation. The Viewer window contains one or more *viewports* where images can be manipulated. Viewports are described on page 12.

You can interact with images as soon as they are visible, while the exam load continues in the background.

Depending on how the exam is opened, the Viewer window may not display the entire exam. To determine which images in an exam have been displayed, use the Preview window. For details, see page 10.

The Browser Window

The Browser window provides a flexible work area for exams that do not lend themselves to display with a hanging protocol. To load an open exam into the Browser window, go to the Preview window and double-click any thumbnail image from that exam.

The Browser displays automatically when images are loaded into it from the Preview window. It can also be displayed (if loaded) by clicking  (the same button used to open the Preview window).

Like the Viewer, the Browser window contains one or more *viewports* where images can be manipulated. Viewports are described below.

Images and Viewports


The Viewer, Browser, and other image-oriented windows are made up of one or more *viewports*. A viewport can contain one or more exams, part of an exam (such as a series), or a single image.

The viewport title bar displays the case number, exam status¹, exam date, and series ID, for the images in the viewport.

The viewport contents title bar displays the number of images, series or sequences, and exams in the viewport.

The viewport info area displays information about the active image in the viewport.


If there are multiple images in a viewport, the active layout dictates if images are displayed 1-up (stacked) or in one or more rows and columns (tiled). In the Viewer and the Browser windows, the layout of each viewport can be changed independently. For details, see page 19.

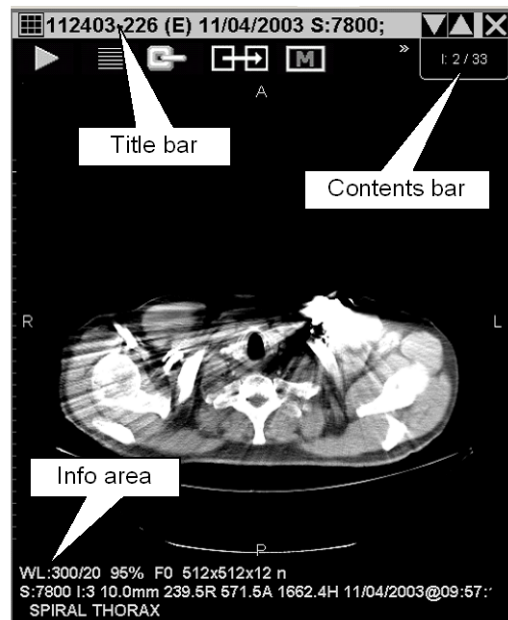

¹ E = examined, I = interpreted, C = complete.

Navigating in Viewports

In a viewport, the Contents bar and tick marks indicate if there are multiple images present, and indicate your relative position in the group of images.

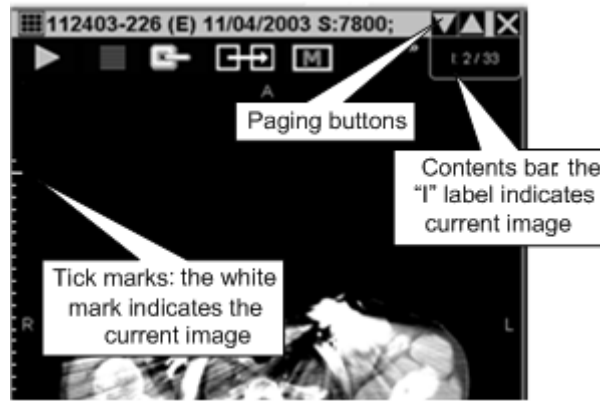


In a viewport that contains multiple images, you can do any of the following to display each image:

- Roll the scroll wheel of your mouse up or down while pointing to the viewport to step through images one at a time.
- Drag up and down using the scroll wheel (or middle mouse button) to scroll rapidly.
- Click the paging buttons located near the top of the viewport. A “page” is based on the current layout (number of visible images) in the viewport.

If a viewport contains multiple exams or multiple series, only one exam/series can be active at once. Other exams or series are considered hidden. The Contents bar indicates if hidden exams or series are present.


To display a hidden exam or series, click on the **Ex** or **S** label on the Contents bar. Then click the item you want to display.

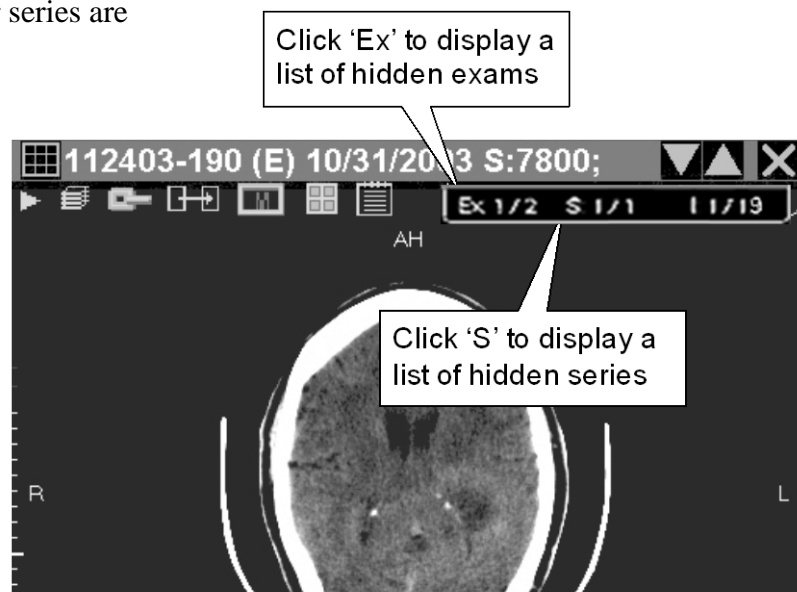


NEW IN 115 > **Conditional Indicator Icons**

VistARad places indicator icons in the upper-right corner of images to alert you to certain conditions. These will appear in any viewport, regardless of the viewport's parent window.

Image Compression Alert


VistARad indicates a compressed image by displaying the Compression Alert icon . Right-clicking on the icon displays a context menu with two options: Clicking **Display Compression Details** opens the Display Data tab of the Image Detail window. Clicking **Hide Icon** will hide it.

VOI LUT Indicator

VistARad indicates that an image has a Value Of Interest Look Up Table applied by displaying the  icon, imprinted with the letters 'LUT' in the upper-right corner of the image. By default, VistARad displays images with the first embedded Value Of Interest Look Up Table applied. Right-clicking the icon displays a context menu with up to three options.

For more details, refer to the *VistARad User Guide*, "Using Conditional Indicator Icons."

Navigating with Scouts

Scout (localizer) images, if present, load automatically into the Scout Image window when an exam is opened. To display the Scout Image window, click  in the Viewer toolbar.

Scout images may load into a viewport in the Viewer if so directed by the hanging protocol in use.

In the Viewer, you can generate a scout image if the displayed exam contains images from intersecting planes. To generate a scout, select the image you want to use, right-click, and then click **Create Scout**. This adds the scout image to the Scout Image window.

VistARad projects cross-referencing slice lines on all applicable cross-sections of simultaneously displayed image sets. VistARad synchronizes them to the stack position of the active viewport. Changing the active viewport re-applies and re-synchronizes all reference slice lines. This is the default behavior, which can be changed from the context menu accessible from the right of the Scout Image window button.

NOTE This user preference setting persists until changed, even after VistARad is closed.

NOTE When the Show X-Ref Slice Lines menu item is unchecked, slice lines appear only on the Scout Image window. When the menu item is checked, slice lines appear on both VistARad Viewer and the Scout Image window.


An illustration of the context menu appears below.



Navigating between Patients

Except for the Manager, all VistARad windows are designed to display information for only one patient at a time. When exams for multiple patients are open, only exams related to the active patient are visible.

All image-related windows include the **Active Patient** button in their title bars. The **Active Patient** button displays the name, SSN, age, and sex of the patient associated with the currently displayed exam.

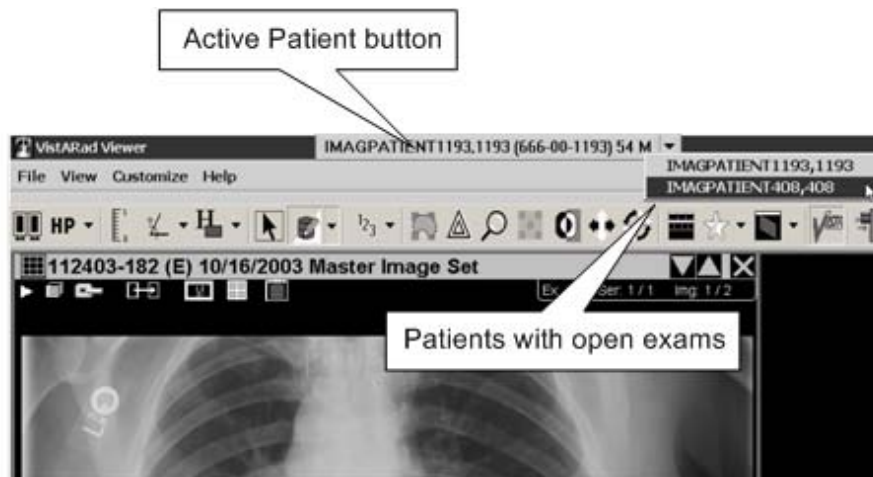

When exams for multiple patients are open, you can click the **Active Patient** button and use a drop-down list to switch between each patient's exams. Switching to a different patient updates all windows in VistARad.


Working with Images


Adjusting Images

The most commonly used tools (pan, scale, window/level) are always assigned to specific buttons on your mouse. You can also temporarily assign any of the standard manipulation tools to the left button of your mouse.

Using Built-In Pan, Scale, and Window/Level


- 1 Point to the image you want to change.
- 2 Click the appropriate mouse button and drag the mouse.

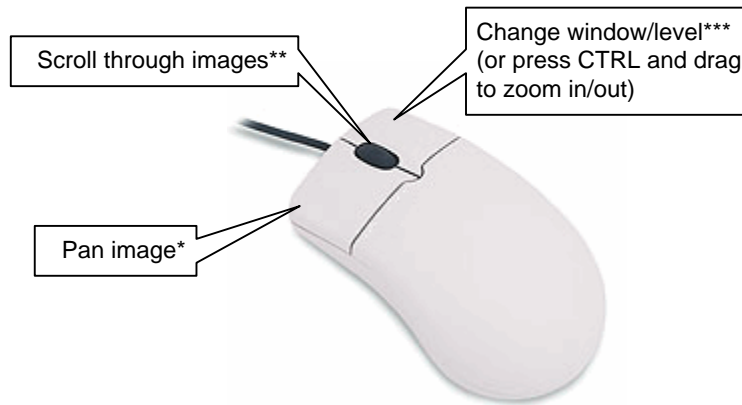







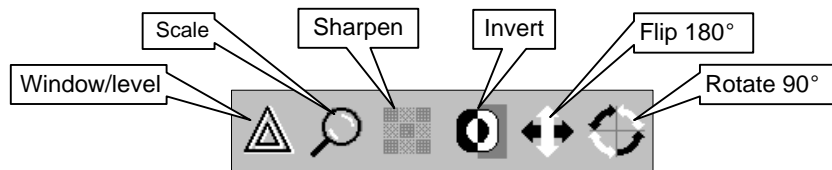


- * Pan is the default operation, and is active when the mouse pointer looks like . See the next section for details.
- ** Scrolling is used for viewports that contain more than one image. See page 13 for more details.
- *** Window/level is the default operation. Settings for the right mouse button can be changed using the options under **View | Settings | Mouse**.

Using Image Manipulation Tools

- 1 Go to the toolbar at the top of the window and click one of the following tools. You can also right-click an image and use the shortcut menu.



- Point to the image you want to work with. The mouse pointer changes, showing the “active area” where the tool can be used.
- Depending on which tool you have selected, do one of the following:

Tool	Pointer	Point to image, then...
Window/level		Drag up or down to change window; drag left or right to change level.
Zoom in/out		Drag up or left to increase zoom; drag down or right to decrease zoom.
Scale image to 100%		Turn on scale tool, then click in upper left part of image.
Scale image to fit viewport		Turn on scale tool, then click in upper middle part of image.
Scale image to specific size		Turn on scale tool, then click in upper right part of image. Choose a scale option from the menu that displays.
Sharpen		Drag up or left to sharpen; drag down or right to smooth.
Invert		Click to invert.
Flip		Click on top part of image to flip vertically; click on bottom to flip horizontally.
Rotate		Click on left side of image to rotate 90° counterclockwise; click on right side to rotate 90° clockwise.

- The tool remains active until disabled. You can change other images, select a different tool, or disable the tool by right-clicking once.

Using Arrow Keys for Precise Control

When you need to make precise window/level, scale, or sharpen adjustments, you can use the arrow keys.

- In the VistARad Settings dialog (**View | Settings**), go to the Mouse/Shortcut tab and make sure the **Enable arrow keys for image adjustments** check box is checked.
- Turn on the window/level, scale, or sharpen tool (assign this tool to the left mouse button as described in the previous section).

- 3 Drag the mouse to make initial rough adjustments (this step can be skipped for the Sharpen tool).
- 4 Use the arrow keys as follows to make precision adjustments:


Shortcut	Description
→ or ↑	Increase window/level, scale, or sharpness (coarse)
CTRL + → or CTRL + ↑	Increase window/level or scale (fine)
← or ↓	Decrease window/level, scale, or sharpness (coarse)
CTRL + ← or CTRL + ↓	Decrease window/level or scale (fine)



Tip For a complete list of keyboard shortcuts and shortcut-related options, see the VistARad Help menu.

‘Apply To’ Settings

Usually changes to window/level, scale, etc., affect all images in a viewport. You can change this behavior and make changes affect only the selected image.

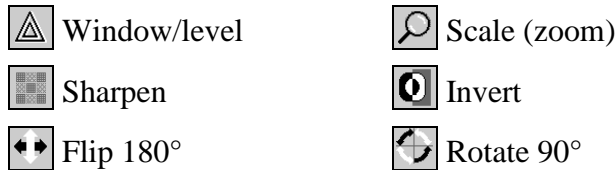
- 1 Click the tool for the property you want to change Apply To settings for:



- 2 In the viewport containing the image you want to change, click the **Apply To** icon.
 - When the **Apply To** icon looks like , your change is applied only to the selected image.
 - When the **Apply To** icon looks like , your change is applied to all the images in the viewport.
 - You can set the default ‘Apply To’ behavior using the options under **View | Settings | Viewport**. (Note that Apply To settings defined in a hanging protocol overrides the settings in this tab.)

Changing Layout in a Viewport

In a viewport, images can be arranged 1-up (stacked) or in multiple rows and columns (tiled). In the Viewer and Browser windows only, you can change viewport layout as follows:

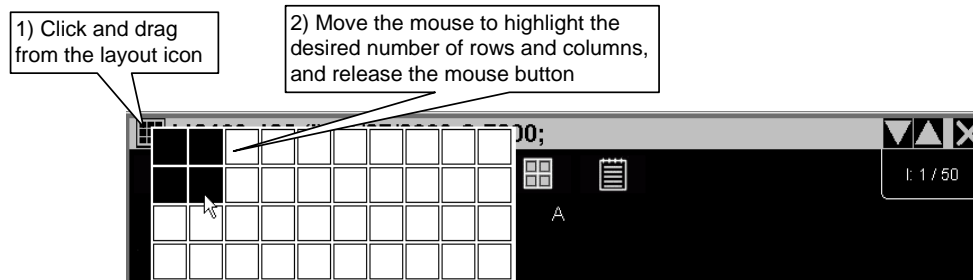


Using Full-Screen View


In the Viewer window only, you can double-click an image to expand it to fit the size of the current monitor. While full-screen view is active, you can change the current image (window/level, flip/rotate, etc.), scroll to other images, or use the cine feature.

If viewport navigation shortcut keys are enabled, you can also press <F> to turn full-screen view on or off. See page 17 for steps to enable shortcut keys.

Changing Layout in a Window

In the Browser, Scrapbook, and Scout windows, you can change window layout as follows:

- 1 Click  and drag down using the mouse.
- 2 In the box that displays, move the mouse to highlight the rows and columns you want to set the layout to.
- 3 When the desired number of rows and columns are highlighted, click the left mouse button.

Tip Click  to switch back and forth between 1-up and the last selected layout.

Note In the Viewer window, the arrangement of viewports is dictated by the current hanging protocol and template.

Manipulating Image Sets

An image set (the active group of images in a viewport) can be moved, or cloned. You can also clear a viewport without closing the associated exam.

Moving an Image Set

In the Viewer window, you can move any image set to a different viewport by dragging the title bar of one viewport into a different viewport.

- If the target viewport in the Viewer is empty, the images being moved are shifted to the target viewport.
- If the target viewport in the Viewer contains a single image set, your user settings determine if the contents of the two viewports are swapped, or if the images being moved replace the images in the target viewport.¹
- If the target viewport in the Viewer contains multiple image sets, you cannot move more images into that viewport.

In the Browser window, you can move image sets from one viewport to another by dragging the title bar of the viewport you want to move.

- If the target viewport in the Browser is empty, the image being dragged is moved to the last position in the Browser window (where images wrap from left to right, then top to bottom).
- If the target viewport in the Browser is occupied, the image being dragged is inserted into the target cell and the pre-existing image set is shifted to the left.

Cloning an Image Set

In the Viewer window only, you can copy the images in one viewport into another (empty) viewport. The resulting ‘clone’ can be manipulated independently of the source images.

- 1 Point to the title bar at the top of the image set you want to clone.
- 2 Using the right mouse button, drag the images to an empty viewport. A popup menu displays when you complete the drag.
- 3 Click the **Clone** option from the menu that displays.

¹ To set “swap” or “replace” as the default behavior, choose **View | Settings | Viewport** and change the settings in the **Drag and Drop Options** area.


Removing an Image Set

To remove images from a viewport, click  in the upper right corner of the viewport. Note that even when all viewports are emptied using this method, the exam is still considered open by VistARad.

Images can be re-loaded into viewports using the Preview window.

Mensurated Scale

When an image is displayed, a mensurated scale can be displayed to the left of the image in the viewport. This scale signifies the length dimensions of the image. The scale uses pixel size data in the image header. If there is no pixel size data available for the image, you can use the Calibrate tool in VistARad to establish a pixel size. For details, see “Using the Calibrate Tool” in the *VistARad User Guide*.

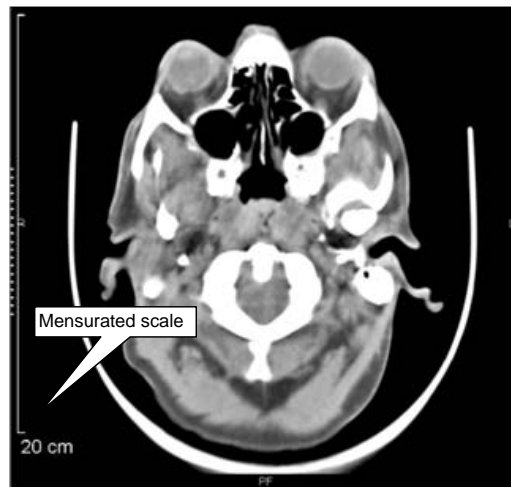


To display the mensurated scale:


- 1 With an image in the viewport, right-click to display the Context menu.
- 2 Click the Mensurated scale option from the menu. The scale will display to the left of the image.

To remove the mensurated scale from view:

- 1 Right-click the image to display the Image Context menu,
- 2 Click the Mensurated scale option, and the scale will no longer be visible.


Annotations

NEW IN 115 > You can add annotations to images displayed in the Viewer, Browser, or Scrapbook windows. The Line Measurement tool is accessed through its own dedicated button (). For the four other annotation-related buttons, the appearance of each icon varies, displaying whichever tool you have used most recently.

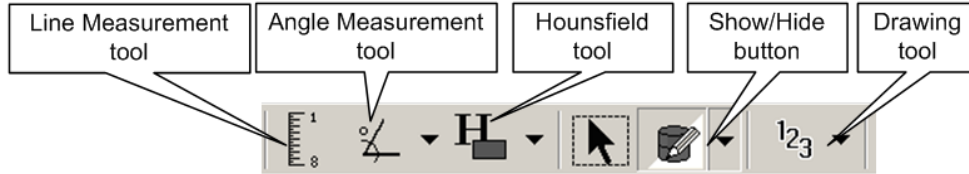





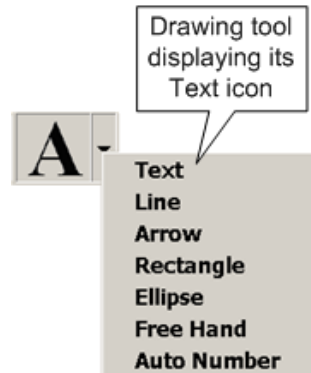


Annotating Images

- 1 Display the image you want to annotate.
- 2 In the Viewer toolbar, click the pulldown arrow to the right of the Drawing tool. Depending on which feature you used last, the icon displays as Text, Line, Arrow, Rectangle, Ellipse, Free Hand, or Auto Number.



- 3 Annotate the image. Steps for each tool are noted below:


Tool	Steps	Pointer
Text	Drag to create the text box, then enter the text.	
Line	Click, then drag. Complete the drag when the line is the desired length.	
Arrow	Click where you want the head of the arrow to display, then drag and adjust as needed.	
Rectangle	Click, then drag. Complete the drag when the shape is the desired size.	

Tool	Steps	Pointer
Ellipse	Click, then drag. Complete the drag when the shape is the desired size, and use the drag handles to adjust.	
Free Hand	Click three or more spots around the desired area, then use the drag handles to adjust as needed.	
Auto Number	In the Auto Number dialog that displays, click the buttons that correspond to the numbering style and starting point you want to use. Then click each point where you want a number to appear.	

- The tool remains active until it is disabled. You can add additional annotations, select a different tool, or right-click once to disable the tool.


Measuring Image Features: Ruler and Angles

To measure length:


- Display the image that contains the feature you want to measure.
- In the Viewer toolbar, click the Length measurement  tool.
- Measure the image feature.



Right-click once to disable the tool. To measure an angle:

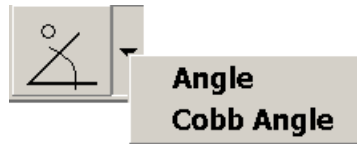- Click the pulldown arrow to the right of the Angle measurement tool. Depending on which feature you used last, the icon displays as either an angle or a Cobb angle.




- Measure the image feature. Steps for each tool are noted below:


Measure	Pointer	Point to image, then...
Length		Click to set the start point of the line, drag the mouse, and release the mouse button when the line is the desired length.

Measure	Pointer	Point to image, then...
Angle		Starting at the vertex, drag the mouse to draw the first line of the angle. The second line is attached to it. Drag either or both lines by their handles to adjust their positions.
Cobb Angle		Starting with the top-most line to be drawn, drag the mouse to create the line. Re-position the lines as needed by dragging the handles.




- The tool remains active until disabled. You can add additional measurements, select a different tool, or right-click once to disable the tool.

Measuring Image Features: Hounsfield Areas

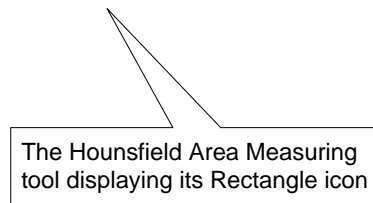- Display the image that contains the feature you want to measure.
- In the Viewer toolbar, click the pulldown arrow to the right of the Hounsfield tool . Depending on which of its three features you have used most recently: the icon displays as Rectangle, Ellipse, or Free Hand.




- Measure the image feature. Steps for each tool are noted below:


Measure	Pointer	Point to image, then...
Rectangle		Click to set the start point of the rectangle, drag the mouse, and release the mouse button when the rectangle covers the desired area.
Ellipse		Click to set the start point of the ellipse, drag the mouse, and release the mouse button when the ellipse covers the desired area. Drag handles as needed to adjust.
Free Hand		Click three or more spots around the desired area, then use the drag handles to adjust as needed.

- The tool remains active until disabled. You can add additional annotations, select a different tool, or right-click once to disable the tool.

Working with Annotations

To change the shape of an annotation, right-click the annotation, choose **Edit Annotation** from the context menu, then drag the handles as desired.


To hide an annotation, click the arrow on the left of  on the toolbar, and choose whether you want just the annotations you have made in that session to display, annotations that have been made in previous sessions, or both.

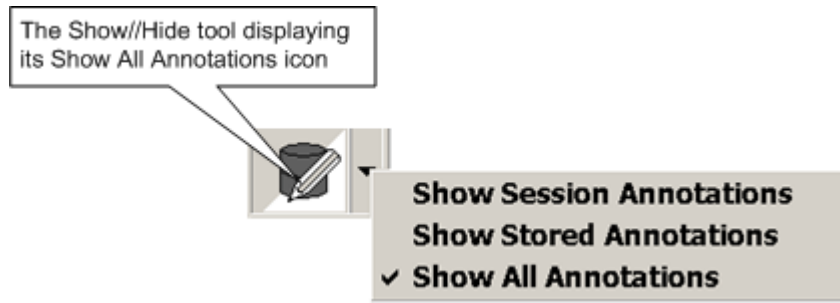

To delete an annotation, right-click it and choose **Delete Annotation**.


Overriding Saved Notations

If you have the MAGJ OVERRIDE ANNOTATIONS security key, you can delete annotations in completed exams, as follows:

- 1 Right-click the completed exam of interest in the Manager window, and choose **Override Annotations**.
- 2 Make any desired additions or other changes to the annotations.
- 3 Click  in the Viewer toolbar.
- 4 Click **Store Annotations in Close Exams/Update Status**.



Key Images

A *key image* is an image that a radiologist has marked as being pertinent to the interpretation of an exam. A key image includes any annotations and display settings (such as window/level) made to the image by the interpreting radiologist.

If an open exam contains key images, they are automatically loaded into the Scrapbook window. If the Scrapbook is not visible, it can be shown by clicking  in the toolbar near the top of the screen.

Marking Images

Marking an image creates an independent copy of the image in the Scrapbook window.



- 1 Open an exam. If you want marked images to be saved as key images, you must have the exam locked in your name.
- 2 Display the image to be marked.
- 3 Click the  icon.
- 4 Continue marking images, or, if you want to work with the image immediately, click  to display the Scrapbook window.

Working with Key Images

You can manipulate and annotate mages in the Scrapbook window.

- If the exam in question is locked, changes to images in the Scrapbook are saved when the exam is closed, and when the status of the exam is updated, images in the Scrapbook become key images.
- If the exam is not locked, changes to the contents Scrapbook are discarded when the exam is closed.

Unmarking Images



To unmark an image and remove it from the Scrapbook, locate the marked image in the Scrapbook and click , or locate the marked image in the Viewer and click .

- If the exam in question is locked in your name, the key image is also permanently deleted (the source image is not affected).
- If the exam is not locked, the key image is retained and displays in the Scrapbook the next time the exam is opened.

Reviewing Online Records

VistARad is typically configured to open requisitions automatically when an exam is opened. You can open other records such as reports or health summaries as well.



Displaying Records

To display a requisition or report for an open exam, click  in an occupied viewport. The requisition displays if the exam is unread. The report displays if the exam has been completed. You can also click, then drag down on the  icon to select either the requisition or the report.

To display a record in the Manager, select an exam. Then right-click the exam and choose an option, or click one of the report-related buttons located under the exam lists in the Manager window.

Working with Health Summaries


The **Health Summary** button is used to access health summary reports.


- If the button includes an asterisk: , clicking the button will open the report you have designated as the default health summary report. Clicking the arrow on the right side of the button will open the Health Summary window.
- If the button looks like this: , there is no default health summary defined, and clicking the button will open the Health Summary window.

The Health Summary window lists any health summary reports that have been selected as preferred reports by the current user.

- To display one of these reports, select the name of the report and click **View Health Summaries**.
- To view a list of all available health summary reports, click **Show Preferences**.
- To edit the user-specific list of preferred reports, click **Show Preferences**, then use the **Add** and **Remove** buttons.
- To select a default report, click Show Preferences, select a report, then click **Set Default**. Click the **Health Summary** button in the Manager to immediately open that report.

Closing Exams

- 1 If VistARad has been integrated with a voice dictation system, and if you have a report open in that system, save or sign the report.
- 2 In VistARad, do one of the following to open the Close Exams / Update Status dialog:
 - Press <CTRL+Q>.
 - Click the  button in the Viewer, Browser, or Scrapbook window.
 - Click **Close Exams** in the Manager window.
- 3 If the exam being closed is locked, and if that exam contains images that have not been viewed,¹ a warning message displays.
 - Click **Continue** to close the exam without displaying all images.
 - Click **Cancel Exam Close** to go back to reviewing images.
- 4 For each exam listed in the dialog, note the values in the **Close?**, **Interpret?**, and **Annotations** columns. Click the values to determine the following:
 - Whether the exam is to be closed.
 - Whether the Interpreted status of the exam has changed (values of N/A cannot be changed).
 - Whether and how annotations, if any, are saved.

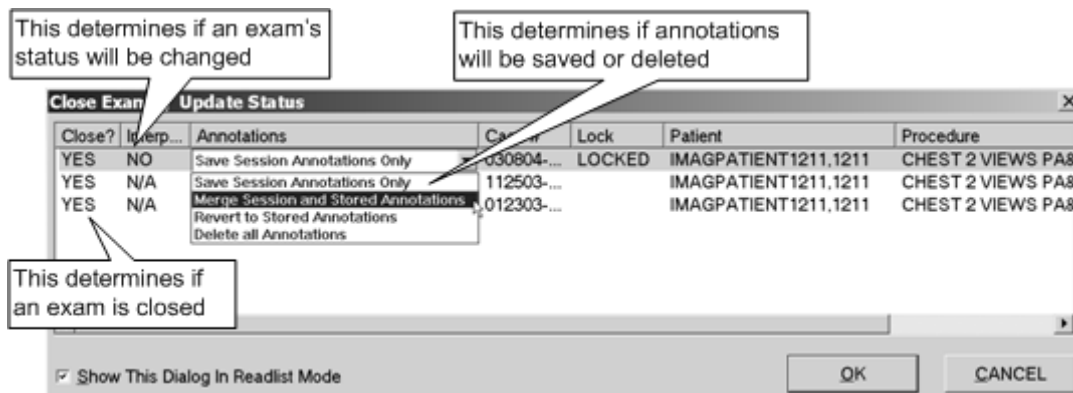

- 5 Click **OK**.
 - When an exam is closed, all images are removed from all windows in VistARad.
 - If **Interpret?** was set to **YES** for a listed exam, that exam's status is updated to indicate that it has been read.

¹ An image set is considered “viewed” if it has been loaded into a viewport and has been “on top” (non-hidden) at some point in the current exam display session.

Hanging Protocols & Templates

This section provides an overview of hanging protocols and templates, and the settings that affect how they are applied.

Template & Hanging Protocol Basics

A template is a specific arrangement of viewports in the VistARad Viewer window. Templates are selected automatically when a hanging protocol is applied to an exam being opened. For more information about using templates, refer to the *VistARad User Guide*.

A hanging protocol automates tasks related to displaying exams. When a hanging protocol is applied, it can:

- Locate priors.
- Load images from current and prior exams into viewports.
- Apply pre-defined image display settings in each viewport.

Hanging protocols are typically selected automatically when an exam is opened. Hanging protocols are matched to exams based on CPT code (procedure), modality type, or both.

You can select a hanging protocol manually before opening an exam. For details, see page 6.

You can also re-display a loaded exam using a different hanging protocol.


Basic Hanging Protocol Settings

The settings under **View | Settings | Hanging Protocol** govern general hanging protocol behaviors. You can:

- Allow or prevent automatic display of priors and related exams for unread exams. There is a similar setting for completed exams.
- Have VistARad notify you if there is a more recent unread exam for a patient than the one you select for display. What qualifies as a more recent unread exam can be based on exact or similar CPT (procedure) matching.

Handling Multiple Matches

If more than one hanging protocol is found for an exam being opened, a dialog listing each of the matching hanging protocols is displayed.

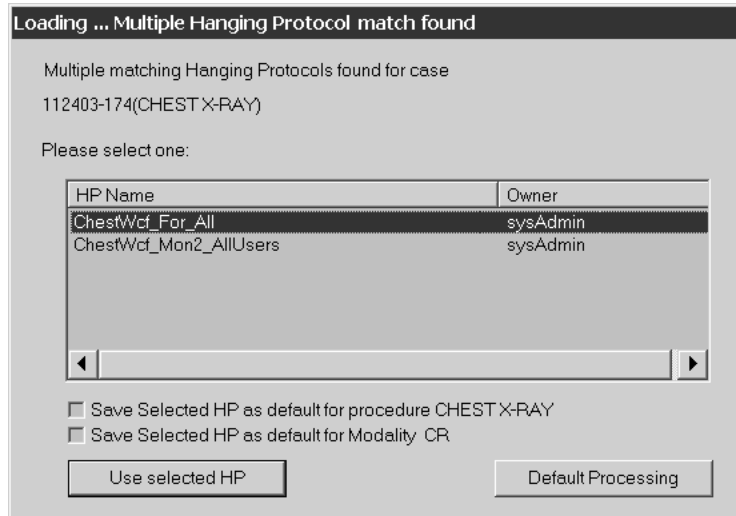

You can choose one of the listed hanging protocols, or you can use default processing (see below).

You can also use one of the **Save...** check boxes in the dialog to make the selected hanging protocol the only hanging protocol used for the current type of exam or modality. (This prevents the multiple match from happening in the future.)

Default Processing

Default processing is used if there are no matching hanging protocols for an exam being opened, or if you explicitly select the **Default Processing** option in the Multiple Hanging Protocol Match dialog.

When default processing is used for an exam:

- Images are loaded in the Preview window and a viewport arrangement (template) is selected in the Viewer.
- No images are loaded into viewports. You can use the Preview window to manually load images into viewports. For details, see page 9.

For details about hanging protocol selection logic and hanging protocols in general, refer to the *VistARad User Guide*.

VistARad and Voxar 3D

Voxar 3D Workstation is a third-party application used to display volumetric images. Voxar and VistARad can be installed and used on the same workstation. When both applications are properly configured, part or all of an exam in VistARad can be opened in Voxar in a single step.

Note It is assumed that the VistARad/Voxar interface has been properly configured, and that the proper version of Voxar is present on the VistARad workstation. For details about configuration, refer to Chapter 3 in the *Vista Imaging System Installation Guide*.

With the proper configuration and security keys, users can also save an image capture from Voxar to the VistA system).

Loading Images from VistARad into Voxar

- 1 In VistARad, open an exam and display the images of interest.
- 2 Right-click the images you want to load into Voxar, and:
 - Choose **View 3D** to load the image set into Voxar.
 - Choose **View 3D all series** to load the exam into Voxar.
- 3 The Voxar software starts automatically and the images load into the Voxar Reading Manager window.
- 4 Manipulate the images as desired in Voxar.

Tip Depending on which security keys you have, you might be able to export, print, or copy images from the Voxar application.

Note The **Finish and Archive** button appears to be enabled even when it is not functional. This button functions only if the ability to save images to VistA has been configured.

- 5 When you have finished, click **Discard and Finish** in the Voxar Reading Manager.

Saving a Voxar Capture to VistA as a New Series

Note This feature is available only if both VistARad and the DICOM Gateway are properly configured.

Note This feature is enabled only for users who hold the MAGJ STORE 3D IMAGES security key.

Before using the following steps, contact your Imaging Coordinator to verify that this feature is available.

- 1 Load images into Voxar from VistARad, and generate the views you want to save.
- 2 When you have created the desired view in Voxar, click **Capture** (located in the lower right corner), then click the view to be captured.
- 3 In the Voxar Reading Manager window, click the Report tab. Then click the thumbnail representing the image you want to save.
- 4 Click **Finish and Archive**. The Voxar windows closes.
- 5 Close and reopen the exam in VistARad. The new image is now available as a separate series.
- 6 After the captured image has been processed by the DICOM Gateway, it is added to the exam as a single-image series. To view the new series, close and re-open the applicable exam in VistARad.

Teaching Files



NEW IN 115 > VistARad provides the ability to create teaching files from images, images sets, and exams. Once uploaded to the Medical Imaging Resource Center (MIRC) server, these files become searchable and available as teaching references for MIRC users.


NOTE It is imperative that images posted to MIRC servers contain no personally identifiable information (PII). Ensuring that images contain no PII is the user's responsibility. VistARad will have already removed any PII from text data. However, burned-in pixel data cannot be removed. Therefore, the user must ensure that there is no PII in the burned-in pixel data of any image uploaded to the MIRC.

NOTE Annotations added to images in VistARad cannot be uploaded to a MIRC; only the images themselves can be uploaded.

NOTE For information about enabling the MIRC interface, see Chapter 3 in the *Vista Imaging System Installation Guide*, or contact your Imaging Coordinator.

Creating Teaching Files

- 1 Open the image, image set or exam in the VistARad Viewer that you wish to make into a teaching file.
- 2 Right-click the image on the screen to bring up the context menu, then click **Add to Teaching Files**.
- 3 Select **Image**, **Image Set**, or **Exam**. This copies the image to the Teaching Files section of the Scrapbook window.
- 4 Repeat the process for any additional images you wish to use; for best results, you should work only with images that are part of the same exam.
- 5 Click  in the toolbar to display the Scrapbook window, and click the Teaching Files tab.
- 6 Click  in the Teaching Files toolbar.
- 7 A warning will display not to upload any files with "burned-in" personally identifiable information. Click **Continue**.
- 8 The Teaching Files window will display. Select the Title box, and enter the name to be used for the teaching file.
- 9 Click the drop-down menu under **Category** and click the desired category.

- 10 Double-click the appropriate descriptive terms in the Findings, and Anatomic Location boxes on the right, and those choices will populate the corresponding boxes on the left.
- 11 Enter any desired free text into the boxes for Diagnosis and Abstract. You can either type or use Copy/Paste to enter text here.
- 12 Click **Send**, or **Send and Close**, and the images will be sent to the teaching folder of your facility on the MIRC server.
- 13 Once you have finished, click  in the Teaching Files toolbar to open the MIRC server Query Page in your browser.

VistARad and Voice Dictation

About the VistARad Dictation Interface

The VistARad dictation interface allows communication with approved voice dictation systems, installed on the same workstation as VistARad, or on a separate workstation. Consult the Imaging Team for a list of approved voice dictation software products.

If the dictation interface is enabled and properly set up, opening and locking an exam for interpretation in VistARad trigger the opening of the exam's report in the dictation software. You can begin dictating a report without having to manually select it ahead of time.



When the VistARad dictation interface is being used, it is the user's responsibility to verify that the proper login is being used to access reports, that the report opened for dictation is the appropriate report, and that report is handled appropriately once dictation is complete.

For information on setting up the VistARad dictation interface, see chapter 3 in the *Vista Imaging System Installation Guide*.

Opening Exams and Reports for Dictation

Before you Begin

- 1 Log in to your voice dictation software (this can either be on the same workstation as VistARad, or on a separate workstation).
- 2 Log in to VistARad.

If you start the dictation software after logging in to VistARad, you need to start the dictation interface manually. To do this, click **Dictation | Establish Dictation Connection** in the Manager main menu.

Opening an Exam and Report for Dictation

- 1 While the dictation interface is active, use the Manager to open an unread exam or to start ReadList.

Note If another report is already open, be sure to save or sign that report before opening additional exams for interpretation.

- 2 As the exam is being opened, the Dictation dialog displays. In the **Dictate?** column, click the YES/NO value to set it as desired.

- Choose YES if you want VistARad to send the case ID to the dictation software (which in turn triggers the display of the associated report).
- Choose NO if you want to open the exam without opening the associated report.

Warning Do not set **Dictate?** to YES for multiple exams unless your Imaging Coordinator has verified that the dictation software can handle multiple case IDs.

- 3 Click **OK**. The dictation software opens the report for the exam.

Note When you go to close an exam that is locked and has a report open for dictation, the value for **Interpret?** in the Close Exams/Update Status dialog defaults to YES. This is based on a user preference in the **Manager | General** tab in the VistARad settings dialog (**View | Settings**).

Opening a Report (only) for Dictation


To open a report in your dictation software via VistARad's dictation interface, right-click any exam in an exam list, then click **Dictate**. Note that:

- This neither opens nor locks the exam. To open the exam itself, select it and click **Open**.
- You are not asked to confirm the operation (the Dictation dialog does not display).
- This can be used for any exam, regardless of the status of the exam.

Remote Data/Image Views

You can use VistARad to view images and reports for radiology exams stored at any remote VA site. You can also view exams stored at DoD medical facilities for VA/DoD shared patients.


When the Patient Exams list is displayed in VistARad, remote sites where the patient has been treated are shown as buttons at the top of the list. Clicking one of the buttons adds exams (if any) from the named site onto the Patient Exams list, and re-sorts the list to show all exams in chronological order.

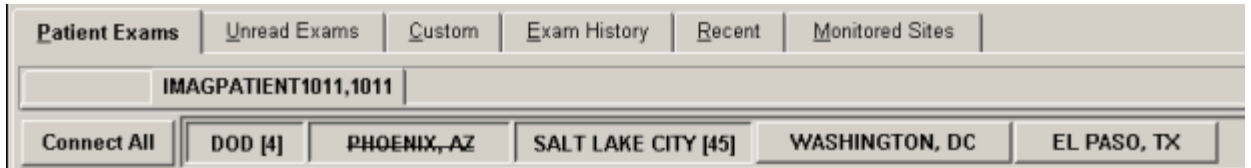

Remote exams shown in the Patient Exams list can be opened for image review, and reports and requisitions can also be displayed. (Note that for DoD exams, images and reports are accessible, but requisitions are not.) The site-local VIX handles retrieval and caching automatically.

When a patient might have remote exams available, based on information from the Master Patient Index, VistARad displays the names of the relevant remote sites on buttons within the Patient Exams tab. Initially, data from the remote sites is not retrieved. To retrieve the data:

- 1 Click the button for the site. This will accomplish the following:
 - Initiates a connection to the remote site. If the site is unavailable, the name in its button will be displayed with a strikeout line through it.

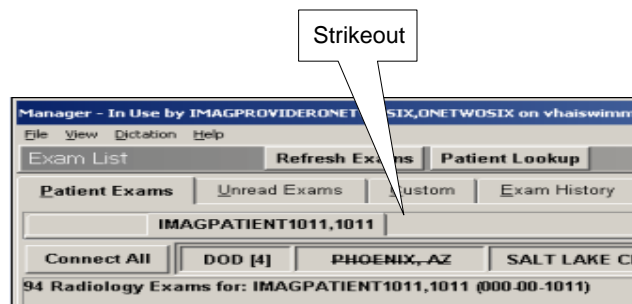

- Loads any available studies into the exam list.
- Updates the label of the button with the number of exams at that site, displayed to the right of its name in square brackets [3].

- 2 Click “Connect All” to automate the steps above for all available sites. The exam list will refresh as the exam list data from each site becomes available.
- 3 Once the data from all remote sites has finished loading, you can begin working with the consolidated exam list.

Remote exams listed in the Manager are available for all VistARad operations available to the current user.

Note DOD studies are consolidated under a single DOD tab, and can be distinguished by a Day/Case column entry starting with “DOD-”:

Day/Case	Lock
121798-29	
121798-29	
DOD-090607-68257027	
DOD-070107-2057319258	
DOD-030707-574831423	
DOD-120806-350785491	
040105-231	
040105-231	